

Certificate of Analysis

Residual Chemicals

Tested by: ISO 17025:2017 accredited, and FDA-registered lab:

Client: Peptide Systems, 50 Iron Point Cir, Ste 140, Folsom, CA 95630

Mass Spectrometry (MS) Residual Chemicals

Product Tested: BPC-157 + TB-500

Lot Number: 250312BT

Analysis Date: 02/11/2025

Method: HPLC-Mass Spectrometry

Instrument: Agilent 6475 Triple Quadrupole LC/MS


Compound Identified: TFA, 2,2,2-trifluoroacetic acid

Molecular Weight Confirmed: Identity Verified

PubChem CID: 6422

TFA not detected, expected retention 0.88 min, conc = 5.26 ppm

PASS, below NOAEL of 10mg/kg/day

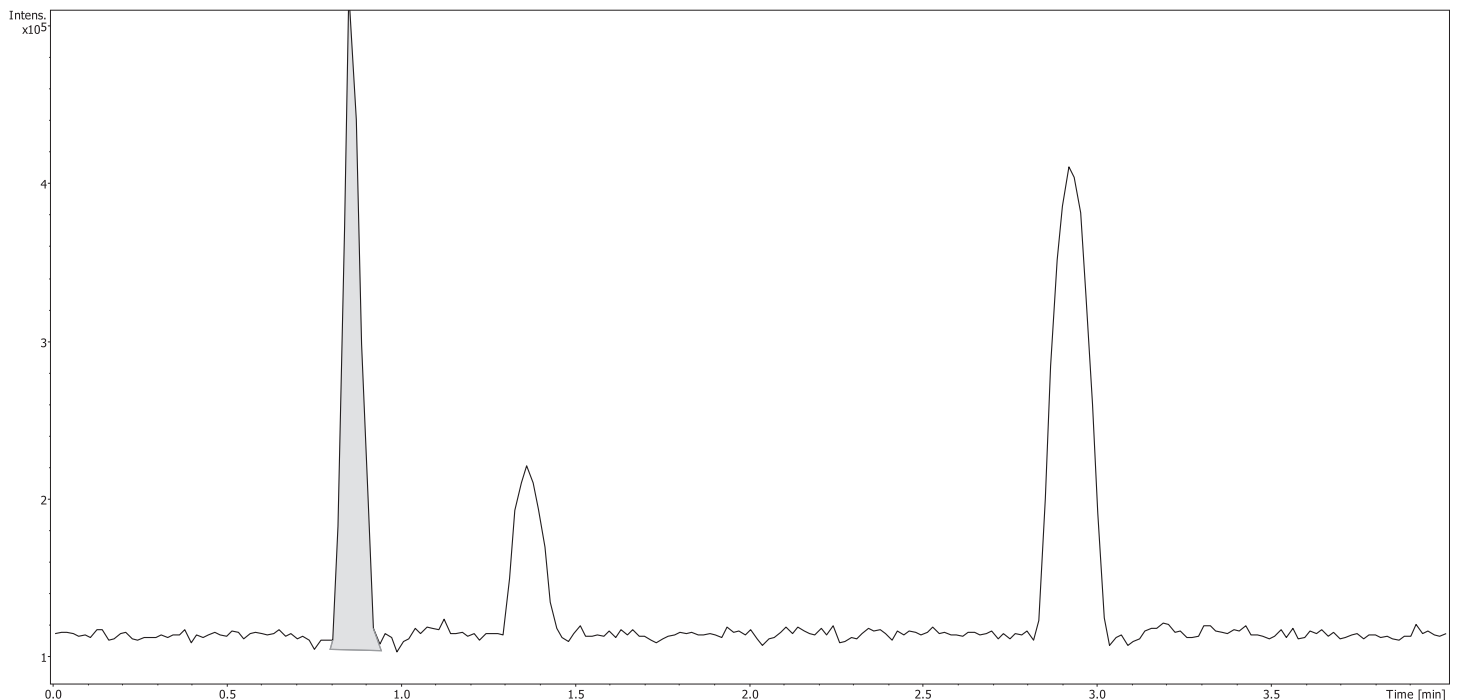

Analytics Technician III

02/11/2025

Date