

Certificate of Analysis

Purity

Tested by: ISO 17025:2017 accredited, and FDA-registers lab: [REDACTED]

Client: Peptide Systems, 50 Iron Point Cir, Ste 140, Folsom, CA 95630

Product Tested: Selank

Lot Number: 240713SN

Date Received: 08/17/2024 **Date Analyzed:** 08/22/2024


Purity: 99.68%

Method: HPLC-UV-MS

Analytical Instrument Model: Agilent 6475 Triple Quadrupole LC/MS

PubChem CID: 11765600

High Pressure Liquid Chromatography (HPLC) UV - MS - Purity Test

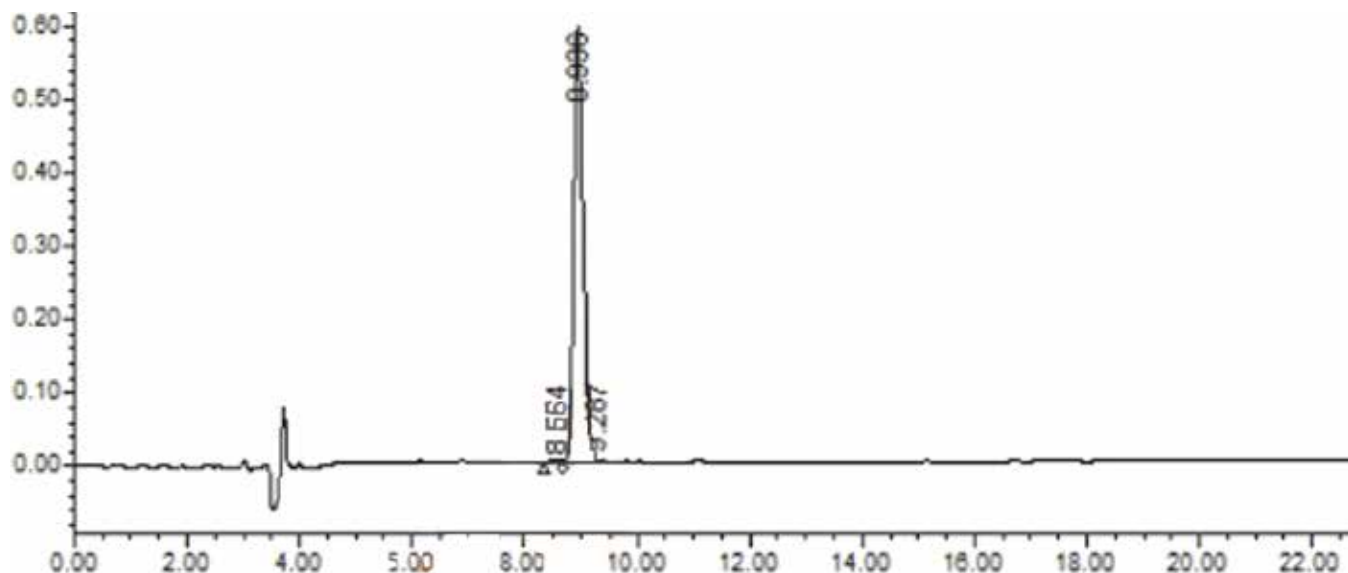

PEAK TIME (min)	AREA	%AREA	
8.48	2.22E+05	99.68	Selank
5.96	1.85E+02	0.02	
5.82	5.46E+01	0.01	
3.83	1.03E+02	0.29	

Combined Purity = 99.68%
Measured Quantity= 10.07mg/vial

Analytics Technician III

08/22/2024

Date