

# Certificate of Analysis

## Purity

**Tested by:** ISO 17025:2017 accredited, and FDA-registered lab:

**Client:** Peptide Systems, 50 Iron Point Cir, Ste 140, Folsom, CA 95630

**Product Tested:** Selank

**Lot Number:** 240713SN

**Date Received:** 08/17/2024 **Date Analyzed:** 08/22/2024


**Purity:** 99.68%

**Method:** HPLC-UV-MS

**Analytical Instrument Model:** Agilent 6475 Triple Quadrupole LC/MS

**PubChem CID:** 11765600

High Pressure Liquid Chromatography (HPLC) UV - MS - Purity Test

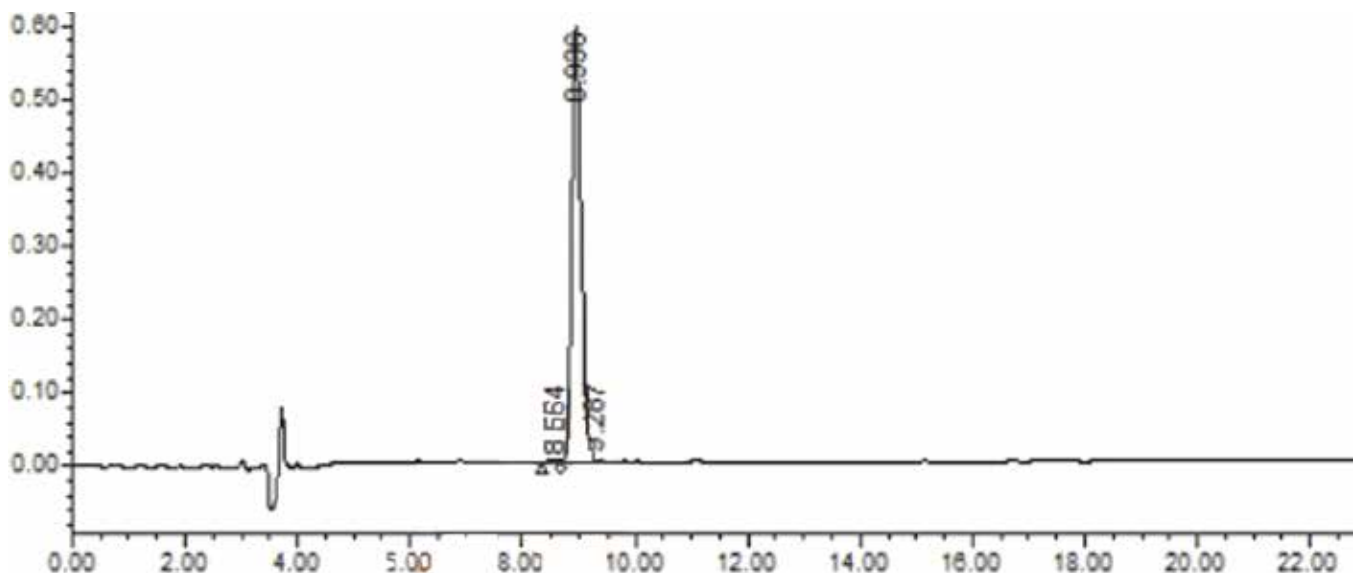

PEAK TIME (min)	AREA	%AREA	
8.48	2.22E+05	99.68	Selank
5.96	1.85E+02	0.02	
5.82	5.46E+01	0.01	
3.83	1.03E+02	0.29	

**Combined Purity** = 99.68%  
**Measured Quantity**= 10.07mg/vial

Analytics Technician III

08/22/2024

Date