

Certificate of Analysis Identity

Tested by: ISO 17025:2017 accredited, and FDA-registers lab: [REDACTED]

Client: Peptide Systems, 50 Iron Point Cir, Ste 140, Folsom, CA 95630

Mass Spectrometry (MS) Identity Test

Product Tested: Semax

Lot Number: 20240724SX

Analysis Date: 08/03/2024

Method: HPLC-MS, molecular wt calculated w monoisotonic m/z from MS


Instrument: Agilent Ultivo Triple Quadrupole LC/MS

Expected monoisotonic mass: 813.92 Da

Measured monoisotonic mass: 813.94 Da

Molecular Weight Confirmed: Identity Verified

PubChem CID: 9811102

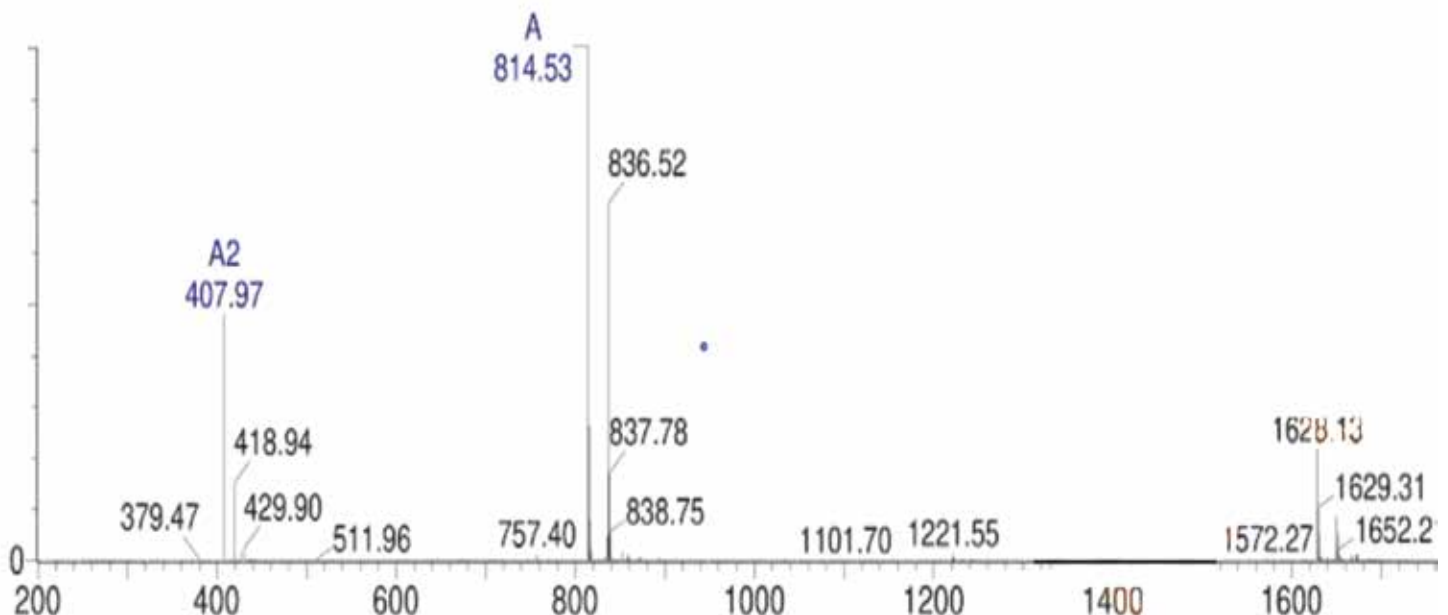

Analytics Technician III

08/03/2024

Date